

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**




## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification <sup>6</sup> : <b>G08B 25/01, A61B 5/00</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 99/45516</b></p> <p>(43) International Publication Date: 10 September 1999 (10.09.99)</p>
<p>(21) International Application Number: <b>PCT/IL99/00108</b></p> <p>(22) International Filing Date: <b>22 February 1999 (22.02.99)</b></p> <p>(30) Priority Data: 123516                      2 March 1998 (02.03.98)                      <b>IL</b></p> <p>(71) Applicant (for all designated States except US): <b>SHL TELEMEDICINE INTERNATIONAL LTD. [IL/IL];</b> Beith Ashdar, Yigal Alon Street 90, 67891 Tel Aviv (IL).</p> <p>(72) Inventor; and (75) Inventor/Applicant (for US only): <b>ALROY, Yoram [IL/IL];</b> Yigal Alon Street 90, 67891 Tel Aviv (IL).</p> <p>(74) Agent: <b>REINHOLD COHN AND PARTNERS; P.O. Box 4060, 61040 Tel Aviv (IL).</b></p>		<p>(81) Designated States: <b>AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</b></p> <p><b>Published</b> <i>With international search report.</i></p>

(54) Title: **EMERGENCY SIGNALING OR DIAGNOSTIC DEVICE**

## (57) Abstract

An emergency signaling or diagnostic device (10), particularly an ECG signaling device (11, 11') embedded within a wallet (35) for signaling a health condition of an owner of the device. The wallet (35) may have embedded therein functions (40) of a cellular telephone and may include a vocalizing unit (16) for producing an acoustic signal representative of the owner's ECG.

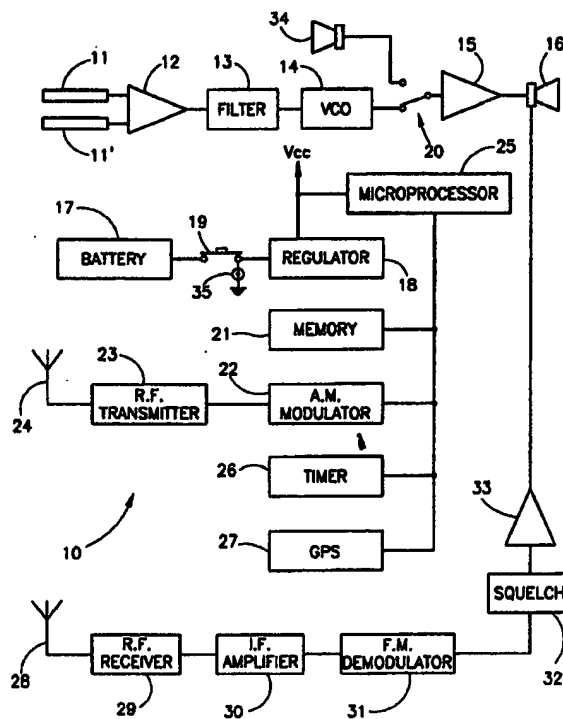

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

## Emergency signaling or diagnostic device

### FIELD OF THE INVENTION

This invention relates to portable electronic instruments for personal use and, in particular, to so-called Personal Emergency Response Systems.

### BACKGROUND OF THE INVENTION

5 It is known that certain people are particularly vulnerable to attack or seizure such as, for example, the elderly and infirm. To this end, it is also known to provide such people with panic alarm devices so that at the onset of an attack, in whatever form that might be, or even in the event of imminent risk thereof, the panic alarm device may be manually operated so as call for help in time of need and inform a central monitoring unit. Upon receipt of a panic  
10 signal, the central monitoring unit may then take appropriate action. Panic alarm devices are, therefore, an important component in the arsenal of those who are vulnerable, thereby providing them with greater security and self-confidence.

Typically, such panic alarms include a manually operated r.f. transmitter energized by a miniature hearing-aid type battery and which, when operated, sends an encoded signal  
15 characteristic of the user. By such means, a remote monitoring unit, upon receiving the encoded signal, knows from where the signal emanated. Most simply, the coding can be by way of modulating an r.f. signal with data representative of the user's personal code so that the received signal is indicative of the sender. A problem associated with such devices is their accessibility. It clearly defeats the whole object of the device if, at a moment of panic, the  
20 device is not readily accessible for actuation and precious time must be wasted in locating it. To this end, such devices are commonly worn as a pendant around the owner's neck, which is liable to be both obtrusive and cumbersome.

It has also been proposed to provide such panic alarms in a wrist-mounted casing including a conventional watch movement, so that the device can double as both a conventional watch and a panic alarm. By such means, the same device serves two functions, thereby increasing its convenience and rendering the panic alarm function completely unobtrusive. In such a device, communication with the remote monitoring unit is effected via  
5 the telephone line and, to this end, there must be provided a base unit connected to the telephone line for effecting wireless communication with the portable device. This is acceptable when the patient is house-bound but is obviously unsuitable for those patients who are generally free to live normal lives but must nevertheless have ready access to the remote  
10 monitoring unit in case of emergency.

Upon effecting communication with the monitoring unit, a patient is frequently required to undertake an interactive dialog with medical personnel at the monitoring unit so as to enable the medical personnel to diagnose the patient's medical symptoms. Since many of those who are particularly at risk suffer from heart-disease, an ECG is usually one of the first  
15 tests which should be carried out. To this end, much effort has been directed to the provision of portable instruments for allowing a patient to carry out an ECG on himself. At their most rudimentary, such instruments comprises a pair of electrodes which are held against a patient's body, usually near his chest to detect an electrical voltage indicative of the electrical activity of the heart. The resulting current waveform response permits partial determination of  
20 the patient's cardiac health. A more detailed determination may be realized by using more than two electrodes and portable devices are known having, for example, twelve electrodes mounted on a common carrier and amenable to placement on a patient's chest area by the patient with minimum effort.

It will be appreciated that no less important than the technical suitability of such ECG  
25 transmitters, is that they must be instantly accessible in a moment of crisis. In the first instance, the required accessibility can only be realized by a portable device. However, experience indicates that this in itself is often not enough. Most people find it difficult to function and to preserve their mental health if they live in constant fear of their mortality. Particularly, those who have a history of heart disease or other serious illness can do without  
30 constant reminders that they might need to perform an instant ECG in the street or elsewhere remote from hospital or home. As a result, there are many who consign the thought to their sub-conscious and it is then but a small step to relegating it to their unconscious altogether.

Such a likelihood would be reduced if the ECG transmitter were not only portable but were so disguised as to be indistinguishable from an everyday item which, in any case, the patient would carry on his or her person. However, the prior art does not seem even to have addressed the problem associated with the almost wanton forgetfulness by the infirm, let  
5 alone propose a solution thereto.

## SUMMARY OF THE INVENTION

This problem is solved in accordance with a broad aspect of the invention by means of an emergency signaling or diagnostic device embedded within a wallet for signaling a health condition of an owner of the device.

10 According to a preferred embodiment, the emergency signaling or diagnostic device is an ECG transmitter having at least two electrodes sewn or otherwise fixed to a surface of the wallet and having controls accessible from inside the wallet. Such a wallet is provided with pockets for accommodating therein cash, credit cards and so on in known manner so that the patient who carries it is psychologically immune from the uncomfortable thought that  
15 anything medical is associated therewith.

In order to allow the patient to relay the ECG signal to a remote monitoring unit, a vocalizing unit may be provided for converting the ECG signal to a representative acoustic signal which can be sent over the telephone to the monitoring unit. Alternatively, the ECG signal may be modulated on to an r.f. carrier signal for direct transmission with the monitoring  
20 unit, thus not requiring that the patient be in ready access with a telephone.

## BRIEF DESCRIPTION OF THE DRAWINGS

A preferred embodiment of the invention will now be described, by way of non-limiting example only, with particular regard a Personal Emergency Response System and with reference to the accompanying drawings, in which:

25 Fig. 1 is a block diagram showing functionally the principal components in a Personal Emergency Response System according to the invention;

Fig. 2 shows pictorially the Personal Emergency Response System of Fig. 1 embedded within a wallet according to a first embodiment the invention;

Fig. 3 shows pictorially an ECG signaling device embedded with a wallet;

Fig. 4 shows pictorially a detail of a wallet serving as a cellular telephone and having embedded therein a Personal Emergency Response System or an ECG signaling device;

Fig. 5 is a flow diagram showing the principal operating steps for use with a microprocessor in the device.

## 5 DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

Fig. 1 shows functionally a Personal Emergency Response System (constituting an emergency signaling device) depicted generally as 10, comprising a portable ECG signaling device having a pair of electrodes 11 and 11' for placing against a patient's bare chest and being coupled to an amplifier 12. The amplifier 12 is coupled to a filter 13 whose output is fed  
10 to a voltage controlled oscillator (VCO) 14 for converting the amplified and filtered ECG signal to an equivalent variable frequency voltage. The VCO 14 thus constitutes a frequency modulator for converting the analog ECG signal to a representative frequency signal centered around 1700 Hz and frequency modulated by the patient's ECG signal. The variable frequency voltage is fed via a first pole of a selector switch 20 to an audio amplifier 15 whose  
15 output may be fed to a loudspeaker 16, which together constitute a vocalizing unit for converting the ECG signal to an equivalent acoustic signal which may be fed over the telephone line to a remote monitoring unit (not shown).

The Personal Emergency Response System 10 is powered by means of an internal battery 17 comprising, for example, three CR 32 cells and being connected to a voltage  
20 regulator 18 via a normally open pushbutton switch 19. Depressing the pushbutton switch 19 thus connects a regulated battery voltage to the various components of the ECG signaling device 10 so that a modulated tone representative of an ECG rhythm strip is output by the loudspeaker 16 for so long as the pushbutton switch 19 is depressed. The three cells within the battery 17 may be removably mounted in a casing of the ECG signaling device 10 so as to  
25 be replaceable, or they may be irremovable in which case the ECG signaling device 10 must be discarded when the battery 17 is spent.

A memory 21 is coupled to an a.m. modulator 22 for amplitude modulating data stored in the memory 21 representative of a unique identity code of the patient as well as any other relevant data. By such means, the patient's personal data and identity may be amplitude  
30 modulated on to a carrier signal which is fed to an r.f. transmitter 23 coupled to an antenna 24. The memory 21 thus serves as an encoder for encoding the patient's personal identity

code, it being understood that other encoding means can equally well be employed, such as, for example, DIP switches and so on.

A microprocessor 25 is coupled to the memory 21 for operating in accordance with an instruction set stored therein. A timer 26 (constituting a timer circuit) is coupled to the microprocessor 25 for providing timing signals thereto, the microprocessor 25 being responsive to the instruction set in the memory 21 and to the timing signals received from the timer 26 for terminating operation a predetermined time period after actuation thereof. The microprocessor 25 is further responsive to the timer 26 for initiating transmission with the remote monitoring unit at regular intervals of time so as to send an "I'm alive" signal at regular time intervals. By such means, even in the absence of manual actuation by the patient, the remote monitoring unit may be assured that the device is functional. Preferably, if the battery voltage is low, part of the transmitted signal is encoded so that the remote monitoring unit may be suitably apprised and take remedial action. Alternatively, the low voltage battery signal may be sent independent of the "I'm alive" signal.

It may be desirable for the Personal Emergency Response System 10 automatically to signal to the remote monitoring unit the exact spatial location of the patient so as to allow an ambulance to be dispatched quickly in the event that the patient is unable to speak. To this end, a GPS unit shown functionally as 27 is coupled to the microprocessor 25. The GPS unit 27 constitutes a spatial location determination unit for receiving GPS positional data via the antenna 24 and allowing it to be forwarded to the remote monitoring unit after suitable modulation on to the r.f. carrier signal.

In order to allow for bi-directional communication with the remote monitoring unit, there is further provided a receiving antenna 28 coupled to an r.f. receiver 29 an output of which is fed to an I.F. amplifier 30 whose output is coupled to a f.m. demodulator 31. An output of the f.m. demodulator 31 is fed in conventional manner to a squelch circuit 32 whose output is coupled via a second pole (not shown) of the selector switch 20 to an output amplifier 33 connected to the loudspeaker 16. A microphone 34 may be connected to the audio amplifier 15 allowing the patient to speak to a medical practitioner at the remote monitoring unit and to hear the medical practitioner through the loudspeaker 16.

Referring to Fig. 2, the Personal Emergency Response System 10 is shown accommodated within a wallet 35, the loudspeaker 16 and the pushbutton switch 19 being sewn or otherwise fixed to an outer surface 36 thereof. An inside surface 37 is provided in



known manner with a plurality of pockets 38 for accommodating notes, credit cards and so on. The remaining circuitry is mounted on a flexible circuit board (not shown) which is secured between the outer and inner surfaces 36 and 37 of the wallet 35. The use of a flexible circuit board allows for the wallet 35 to be folded and subject to moderate deformation as  
5 may be applied when the wallet 35 is placed, for example, in a patient's rear trouser pocket and is thereby subject to deformation whenever the patient sits down.

Referring to Fig. 3, there is shown accommodated within a wallet 35 only an ECG signaling device whose electrodes 11 and 11' are sewn or otherwise fixed to a first outer surface 36 thereof. The loudspeaker 16 and the pushbutton switch 19 are mounted within the  
10 outer and inner surfaces 36 and 37 of the wallet 35 so as to be accessible from the outer surface 36. The remaining circuitry is mounted on a flexible circuit board (not shown) which is secured between the outer and inner surfaces 36 and 37 of the wallet 35. In use, and in the absence of the autonomous wireless transmission means constituted by the r.f. transmitter 23 shown in Fig. 1, the patient must first approach a telephone and dial the remote monitoring  
15 unit. Connection having been established, he now places the electrodes 11 and 11' in position and activates the device by depressing the pushbutton switch 19. As noted above, this produces an acoustic signal representative of the ECG rhythm strip and the acoustic signal is transmitted over the telephone line in the usual way.

Fig. 4 shows schematically the wallet 35 having embedded therein an emergency  
20 signaling device and sharing the functions of a miniature cellular telephone. To this end, there is provided an antenna (not shown) in the spine of the wallet. The antenna may be either of fixed, inextendible length or may be telescopic in which case a small part of the antenna may protrude from the wallet to facilitate extraction thereof. A keypad 40 and display (not shown) may be provided on the inner surface 37 of the wallet, these features being well known *per se*  
25 and therefore not requiring further elaboration.

In the event that the emergency signaling device embedded within the wallet 35 is an ECG signaling device, the electrodes 11 and 11' may be fixed to the outer surface 36 of the wallet 35 as shown in Fig. 3. The pushbutton switch 19 may be duplicated by one of the conventional keys, such as the SEND or TRANSMIT buttons of the cellular telephone.  
30 Likewise, the loudspeaker 16 and the microphone 34 may duplicate the conventional components of the cellular telephone.

Fig. 5 shows the principal operating steps associated with the instruction set stored in the memory 21 for controlling the microprocessor 25. The microprocessor 25 is responsive to an interrupt signal that is produced whenever the pushbutton switch 19 is depressed. The interrupt signal is also produced at regular time intervals based on the timing signal produced by the timer 26. When the pushbutton switch 19 is depressed so as to actuate the device, the user identity code stored in the memory 21 is fetched by the microprocessor 25 and fed to the a.m. modulator 22 which modulates the r.f. carrier signal therewith so as to send an a.m. signal via the antenna 24 to the remote monitoring unit. A signal, representative of the voltage of the battery 17, is fed to the microprocessor 25 that determines the condition of the battery therefrom and generates a corresponding battery condition signal. The r.f. carrier signal is frequency modulated with the battery condition signal so as likewise to be transmitted to the remote monitoring unit. It should be understood that the battery condition signal is merely representative of the normal operating condition of the device, it being contemplated that other signals representative of the device status may be measured, thus allowing the r.f. carrier signal to be modulated therewith and providing the monitoring unit with a full picture of the device operability.

Thus, upon the antenna 24 receiving the r.f. signal, the remote monitoring unit determines whether the device status is O.K. and, if not, takes suitable remedial action. In the absence of further pressure on the pushbutton switch 19, a predetermined time interval is measured by the timer 26, when a further interrupt is generated and the cycle repeats.

Preferably, successively depressing the pushbutton switch 19 alternatively actuates and deactuates the device. Likewise, the microprocessor 25 is preferably responsive to the timer 26 for disabling deactuation of the device for a predetermined time period following actuation thereof. For example, following actuation of the device by pressing the pushbutton switch 19, further depression thereof within a time window of three seconds has no effect. Furthermore, preferably deactuation within a predetermined time period is effected by means of sustained pressure on the pushbutton switch 19. These factors may be important when the device is used by the elderly or infirm, so as to guard against the effect of finger shake.

Upon actuating the device, an a.m. r.f. signal is transmitted to the remote monitoring unit where the user's unique identity is decoded. Once communication has been established, the user chooses the correct setting of the selector switch 20 so as to connect the microphone 34 to the amplifier 15. The user may now speak into the microphone 34 so as to frequency

modulate the r.f. signal, the resulting modulated carrier signal being transmitted to the remote monitoring unit. By such means, the user of the device 10 may converse with a medical practitioner situated remotely at the monitoring unit site. Alternatively, when it is desired to transmit the ECG rhythm strip, the selector switch is set to the other position, so as to  
5 connect the VCO 14 to the amplifier 15.

An LED 35 is coupled to the pushbutton switch 19 so as to be illuminated when the pushbutton switch is closed, thereby providing a visual indication of the operation of the device.

It will be appreciated that modifications and variations may be effected to the  
10 preferred embodiments without departing from the spirit of the invention. Thus, for example, whilst the invention has been described with particular reference to a Personal Emergency Response System, it will be understood that such a system contains many features which can be dispensed with if bi-directional communication with the monitoring unit is not required. In such case, for example, a wallet may be provided with only the ECG signaling device and a  
15 transmitter for transmitting the ECG rhythm strip to the remote monitoring unit together with a signal encoding the user's ID and location. If a microphone is provided, then there is no need to encode either the user's ID or location since he can direct the remote monitoring unit as to his identity and whereabouts. Thus obvious design variations can be implemented according to individual requirement.

20 Likewise, different modulation techniques may be employed as are well known in the art. The battery condition signal may be sent together with the "I'm alive" signal or independent thereof, and so on. Other common household articles may be adapted to incorporate therein the ECG signaling device or, indeed, other electronic devices so as to serve a dual purpose, thereby increasing the likelihood that their owner will wish to make use  
25 thereof. It will also be understood, as noted above, that whilst the ECG signaling device shown in the preferred embodiment has two electrodes, this is not a feature of the invention which contemplates the use of ECG signaling devices having more than two electrodes. It will also be appreciated that it is immaterial whether the ECG electrodes are fixed to an interior or exterior surface of the wallet.

**CLAIMS:**

1. An emergency signaling or diagnostic device (10) embedded within a wallet (35) for signaling a health condition of an owner of the device.
2. The device according to Claim 1, wherein the wallet (35) has embedded therein  
5 functions (40) of a cellular telephone.
3. The device according to Claim 1 or 2, comprising an ECG signaling device (11, 11').
4. The device according to Claim 3, including a vocalizing unit (16) for producing an acoustic signal representative of the owner's ECG.
- 10 5. The device according to any one of Claims 1 to 4, being a Personal Emergency Response System (10).
6. The device according to any one of Claims 1 to 4, for relaying data associated with the owner of the device to a remote monitoring unit, the device comprising:  
an r.f. transmitter (23) coupled to an antenna (24) and a battery (17) and  
15 mounted within a casing (36, 37) of said article,  
an identification unit (21, 27, 34) for relaying a personal identity and spatial location of the owner of the device, and  
a modulator (22) coupled to the r.f. transmitter (23) for modulating an r.f. carrier signal with said data.
- 20 7. The device according to Claim 6, wherein the identification unit comprises:  
a processor (25),  
an encoder (21) coupled to the processor (25) for encoding the personal identity of the owner of the device, and  
a spatial location determination unit (27) coupled to the processor (25) for providing  
25 a signal indicative of a spatial location of the device.
8. The device according to Claim 6 or 7, further including a visual indication device (35) coupled to the battery (17) via an actuator (19) for providing a visual indication of an actuation of the device.
9. The device according to Claim 6, wherein:  
30 the identification unit comprises a microphone (34) for receiving a voice signal for allowing the owner of the device to recite his identity and/or spatial location.

10. The device according to Claim 6, including a processor (25) which is responsive to a battery condition signal representative of a condition of the battery (17) for modulating the r.f. signal with said battery condition signal so as to inform the monitoring unit accordingly.
11. The device according to Claim 10, wherein the processor (25) is responsive to a  
5 voltage of the battery being lower than a predetermined threshold for automatically transmitting the r.f. signal.
12. The device according to any one of claims 7, 10 or 11, further including a timing circuit (26) coupled to the processor (25) for terminating operation thereof a predetermined time period after initiation of the actuator.
- 10 13. The device according to any one of Claims 7, 10 or 11, further including a timing circuit (26) coupled to the processor (25) for transmitting an "I'm alive" signal for relaying to the remote monitoring unit at predetermined intervals of time.
14. The device according to Claim 8, wherein the actuator is a manual pushbutton switch (19).
- 15 15. The device according to Claim 14, wherein successively depressing the pushbutton switch alternately actuates and deactuates the device.
16. The device according to Claim 13, including a manually operated switch (19) for actuating and de-actuating the device and wherein:  
the processor (25) is responsive to the timing circuit (26) for disabling  
20 deactuation of the device for a predetermined time period following actuation thereof.
17. The device according to Claim 16, wherein the processor (25) is further responsive to the timing circuit (26) for actuating only when the manually operated switch (19) is operated for longer than a predetermined time period.
18. The device according to any one of Claims 6 to 17, further including:  
25 a receiving antenna (28) for receiving an r.f. signal from the remote monitoring unit,  
an r.f. receiver (29) coupled to the receiving antenna and having an output fed to an I.F. amplifier (30),  
a demodulator (31) coupled to an output of the r.f. receiver and having an output fed to a squelch circuit (32),  
30 an audio amplifier (33) coupled to an output of the squelch circuit and being connected to a loudspeaker (16).

19. The device according to any one of Claims 6 to 17, including:

a microphone (34) switchably connected to an input of an audio amplifier (15) having a loudspeaker (16) connected to an output thereof for allowing the owner to speak to a medical practitioner at the remote monitoring unit and to hear the medical practitioner  
5 through the loudspeaker.

20. The device according to any one of claims 6 to 19, being mounted on a flexible circuit board.

1/4

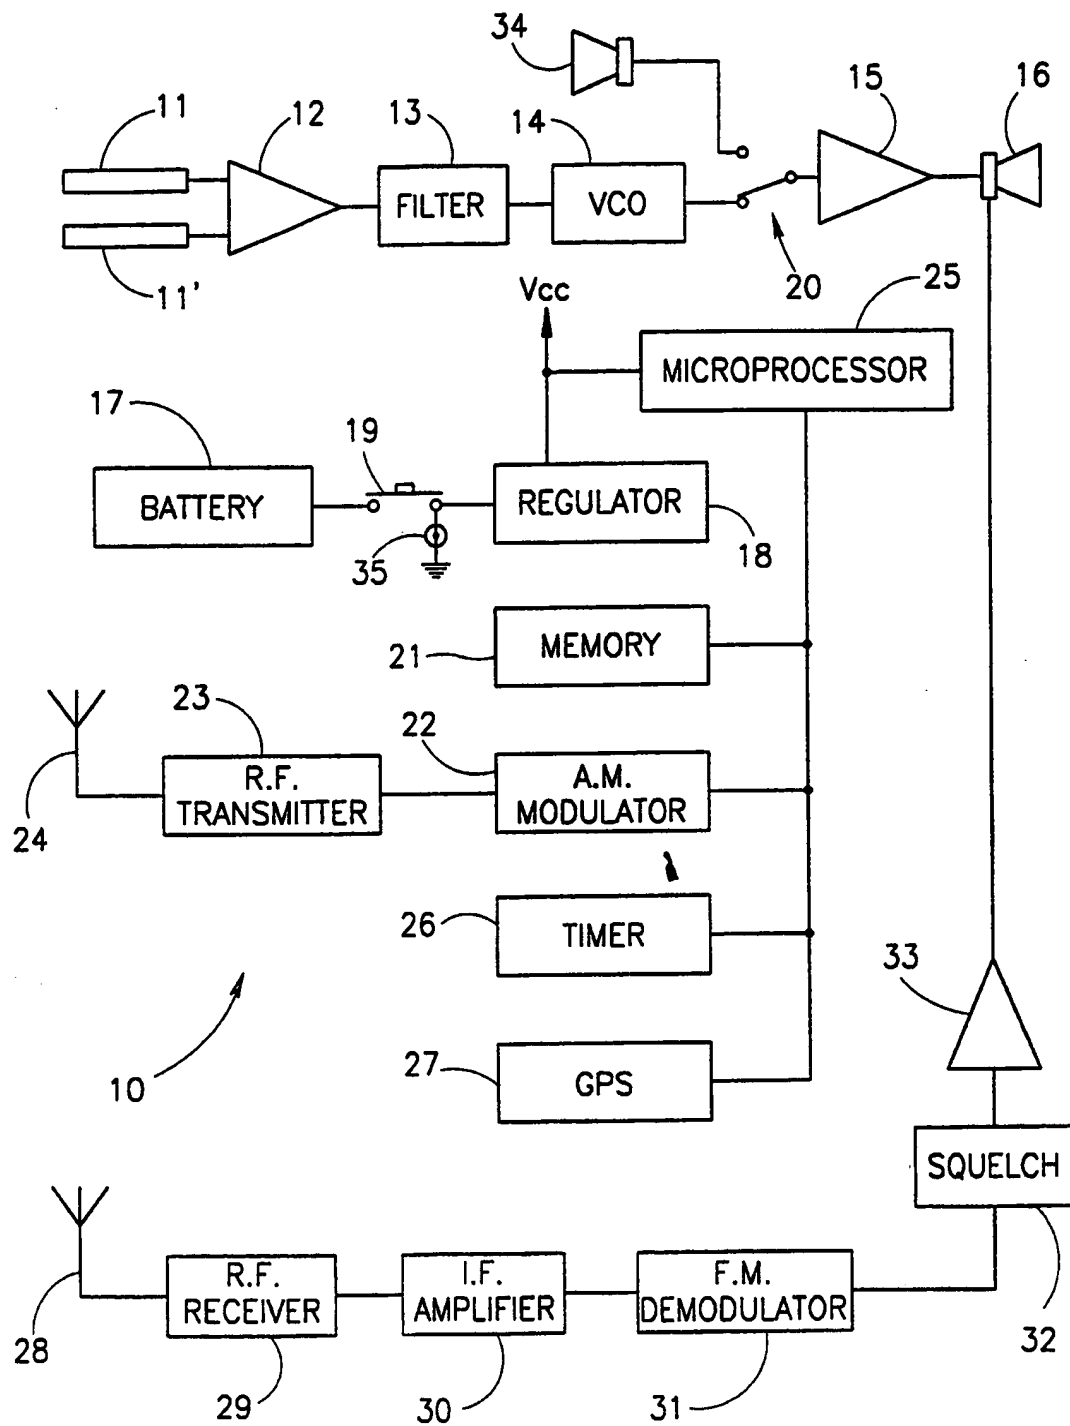


FIG.1

2/4

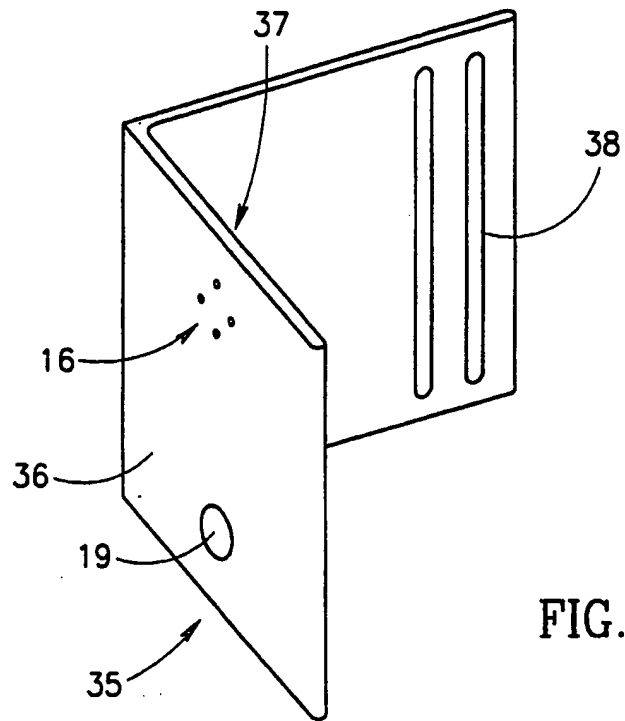


FIG. 2

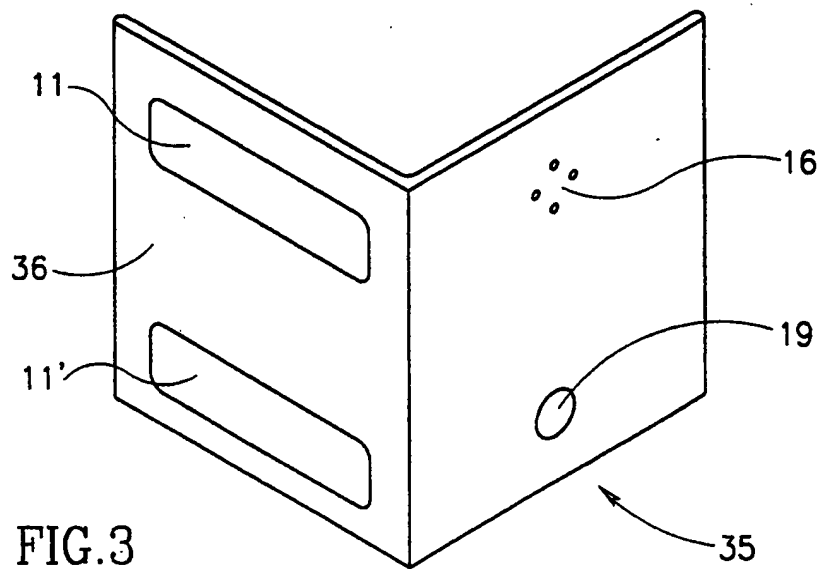


FIG. 3



3/4

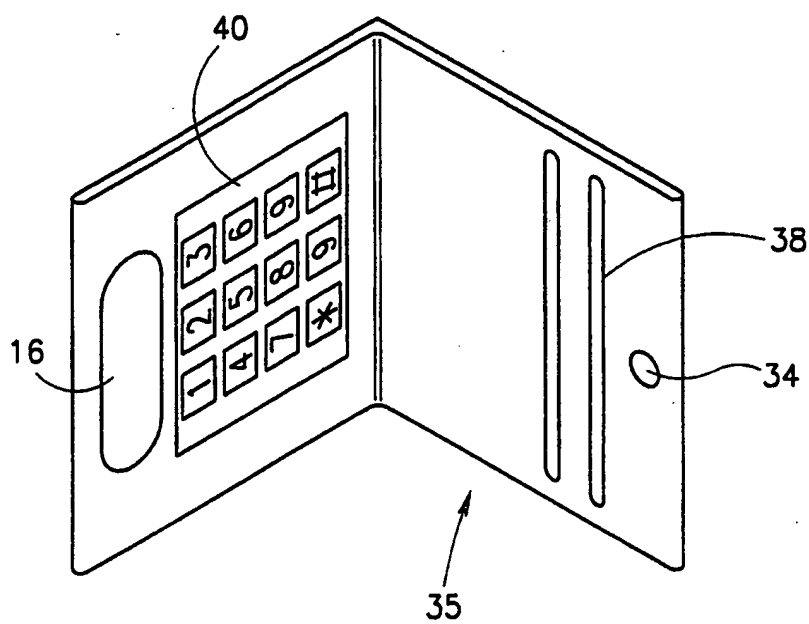


FIG. 4

4/4

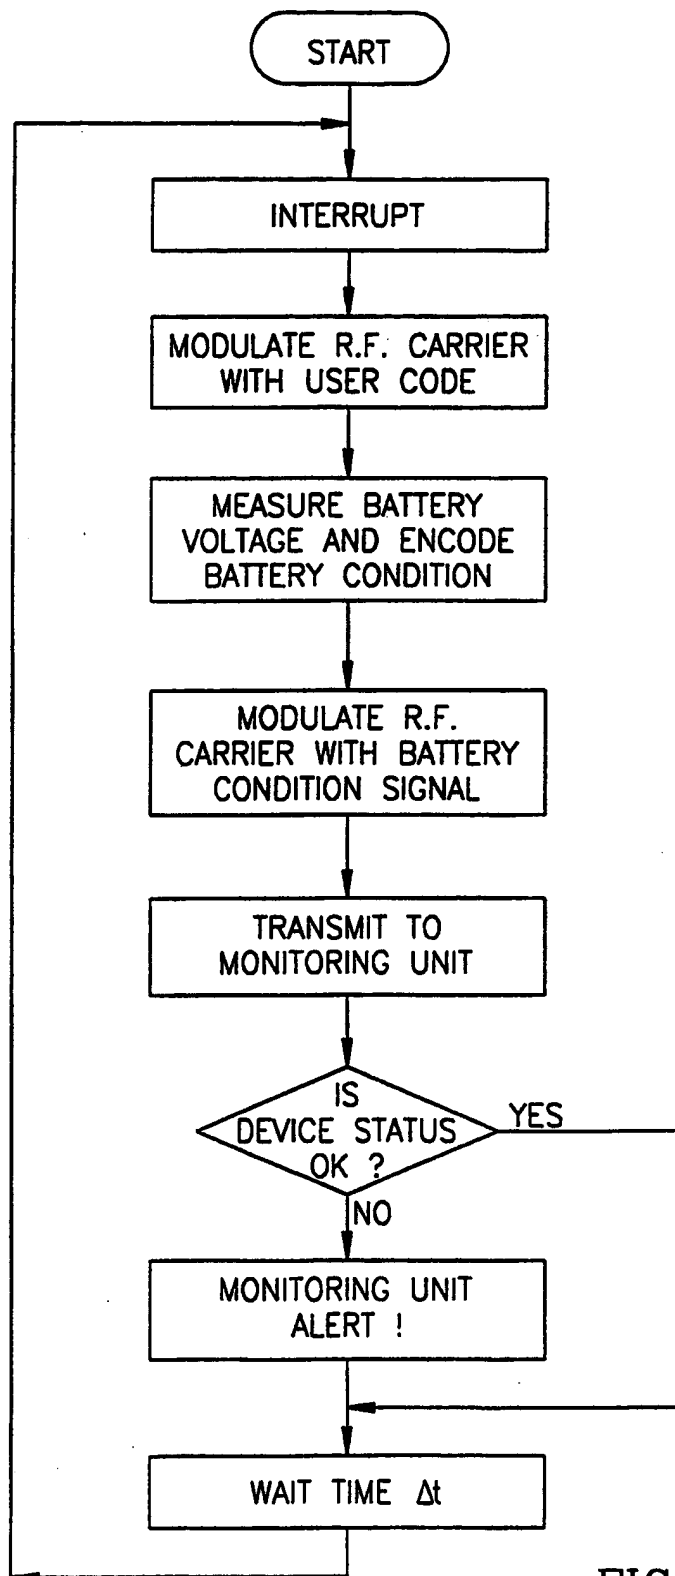


FIG.5

# INTERNATIONAL SEARCH REPORT

Int. Application No

PCT/IL 99/00108

**A. CLASSIFICATION OF SUBJECT MATTER**  
IPC 6 G08B25/01 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G08B A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	GB 2 285 135 A (HEWLETT PACKARD CO) 28 June 1995 see claims ---	1-12, 14-20
Y	US 5 514 862 A (SALZANO DOREEN L) 7 May 1996 see the whole document ---	1,2,6
Y	US 5 058 597 A (FUJII TADASHI ET AL) 22 October 1991 see abstract see column 4, line 22 - line 42; figures 2,3 see column 5, line 27 - line 30 ---	1,20
Y	EP 0 535 629 A (SHACHAL MEDICAL SERVICES LTD ;TADIRAN LTD (IL)) 7 April 1993 see the whole document ---	3-9,14, 18,19
	-/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

\* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

2 June 1999

Date of mailing of the international search report

09/06/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3018

Authorized officer

Reekmans, M

# INTERNATIONAL SEARCH REPORT

Int. l. Application No.

PCT/IL 99/00108

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 87 05137 A (CHAMPION BRUCE) 27 August 1987 see the whole document ---	8,12, 14-17
Y	US 5 162 776 A (BUSHNELL ROBERT A ET AL) 10 November 1992 see claims ---	5
Y	US 4 622 544 A (BIALLY THEODORE ET AL) 11 November 1986 see the whole document ---	10,11
A	GB 2 312 066 A (DRAEGERWERK AG) 15 October 1997 see the whole document -----	1-3,6,7, 18

# INTERNATIONAL SEARCH REPORT

Information on patent family members

Int. l. Application No

PCT/IL 99/00108

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
GB 2285135	A	28-06-1995	DE 4441907 A JP 7234982 A	22-06-1995 05-09-1995
US 5514862	A	07-05-1996	NONE	
US 5058597	A	22-10-1991	JP 2286128 A	26-11-1990
EP 0535629	A	07-04-1993	IL 99620 A	07-10-1994
WO 8705137	A	27-08-1987	AU 7036887 A EP 0258316 A ZA 8701097 A	09-09-1987 09-03-1988 06-08-1987
US 5162776	A	10-11-1992	CA 2072863 A,C EP 0522660 A	10-01-1993 13-01-1993
US 4622544	A	11-11-1986	NONE	
GB 2312066	A	15-10-1997	DE 19614231 A US 5874897 A	16-10-1997 23-02-1999